


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kim DePaola	SPC Number in OTIS:	SPC54509	01-13-16: KD used approved 601-80-074-1CRMU, updated to new component number and made revs per marked up PDF for Crimson PH2 project. 01-13-16 CR signed
Date File Was Last Modified:	01-13-16	Dimension on SPC:	2" x .875"	
2nd Designer review: (layout and requested changes only)	01-13-16 CR	Line Screen:	PMS 185 - 30% using 85 line screen	
PMS Colors Used in File:		Black PMS 185		

601-80-091-1
Red Cells Label



Ortho Clinical Diagnostics
Pencoed, UK

APR 12th Oct 2017

OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kim DePaola	SPC Number in OTIS:	SPC54510	01-13-16: KD used approved 601-80-075-1CRMU, updated to new component number and made revs per marked up PDF for Crimson PH2 project. 01-13-16 CR signed
Date File Was Last Modified:	01-13-16	Dimension on SPC:	2" x .875"	
2nd Designer review: (layout and requested changes only)	01-13-16 CR	Line Screen:	PMS 185 - 30% using 85 line screen	
PMS Colors Used in File:		Black PMS 185		

601-80-092-1
Red Cells Label




Ortho Clinical Diagnostics
Pencoed, UK

12th Oct 2017

OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kim DePaola	SPC Number in OTIS:	SPC54511	01-13-16: KD used approved 601-80-076-1CRMU, updated to new component number and made revs per marked up PDF for Crimson PH2 project. 01-13-16 CR signed
Date File Was Last Modified:	01-13-16	Dimension on SPC:	2" x .875"	
2nd Designer review: (layout and requested changes only)	01-13-16 CR	Line Screen:	PMS 185 - 30% using 85 line screen	
PMS Colors Used in File:	Black		PMS 185	

601-80-093-1
Red Cells Label



Ortho Clinical Diagnostics
Pencoed, UK


PHD An 12th Oct 2017

OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer / Who Last Modified File:	Kim DePaula	SPC Number in OTIS:	SPC54480
Date File Was Last Modified:	01-13-16	Dimension on SPC:	3.486" x 2.181" x 2.75"
2nd Designer review:	01-13-16 CR	Line Screen:	None
(layout and requested changes only)			
PMS Colors Used in File:	Black	PMS 185	Non Varnish

01-13-16 KD used approved 701-85-000-1CRML updated component number and made revs per marked up PDF for Crimson PH2 project.
01-13-16 CR signed

701-80-010-1
Red Cell Carton
France

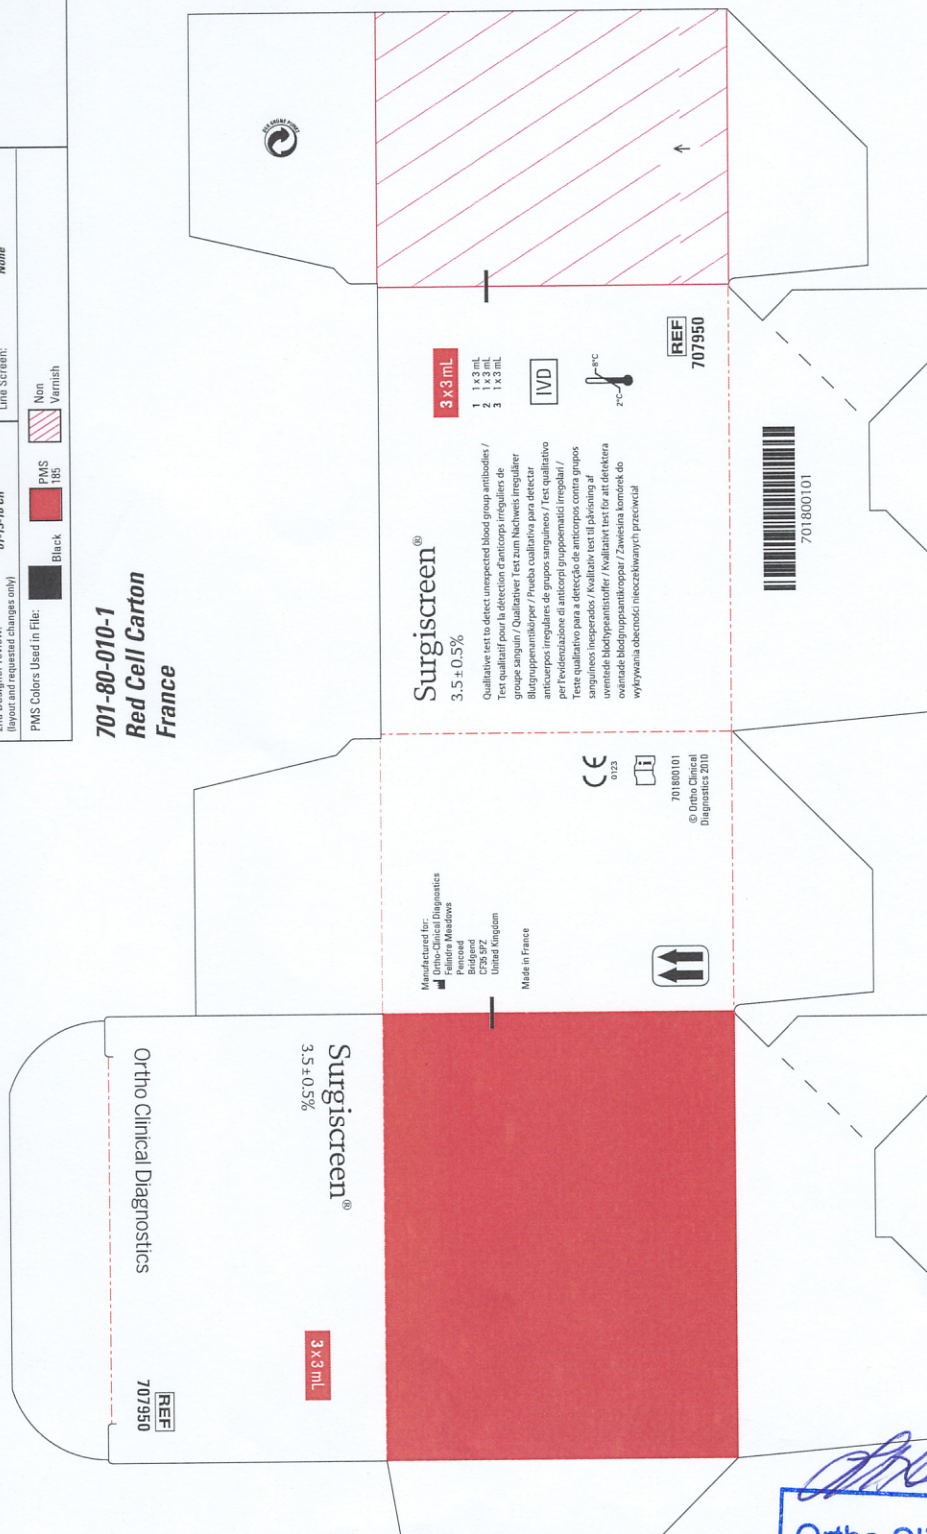

Ortho Clinical Diagnostics
Pencoed, UK

12th Oct 2017