


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File: Kim DePaola	SPC Number in OTIS: SPC54521	01-14-16: KD used approved 601-80-012-1CRMU, updated to new component number and made revs per marked up PDF for Crimson PH2 project. 01-15-16 KT signed.
Date File Was Last Modified: 01-14-16	Dimension on SPC: 2.25" x 1.25"	
2nd Designer review: (layout and requested changes only)	Line Screen: 30% screen of PMS 298 - using 85 line screen	
PMS Colors Used in File:		
 Black	 PMS 185	
	 PMS 298	

601-80-096-1

Red Cells Vial Label



12th Oct 2017


Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kim DePaola	SPC Number in OTIS:	SPC54522	01-14-16: KD used approved 601-80-013-1CRMU, updated component number and made revs per marked up PDF for Crimson PH2 project. 01-15-16 KT signed.
Date File Was Last Modified:	01-14-16	Dimension on SPC:	2.25" x 1.25"	
2nd Designer review: (layout and requested changes only)	01-15-16 KT	Line Screen:	30% screen of PMS 298 - using 85 line screen	
PMS Colors Used in File:	Black		PMS 185	
			PMS 298	

601-80-097-1

Red Cells Vial Label




12th Oct 2017
Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File: <i>Kim DePaola</i>	SPC Number in OTIS: <i>SPC54523</i>	01-14-16: KD used approved 601-80-014-1CRMU, updated component number and made revs per marked up PDF for Crimson PH2 project. 01-15-16 KT signed.
Date File Was Last Modified: <i>01-14-16</i>	Dimension on SPC: <i>2.25" x 1.25"</i>	
2nd Designer review: (layout and requested changes only)	Line Screen: <i>30% screen of PMS 298 - using 85 line screen</i>	
PMS Colors Used in File:		
 Black	 PMS 185	 PMS 298

601-80-098-1

Red Cells Vial Label



12th Oct 2017
Ortho Clinical Diagnostics
Pencoed, UK

Designer: Who Last Modified File:	Kim DePaola	SFC Number in OTIS:	SPC54462
Date File Was Last Modified:	01-14-16	Dimension on SFC:	2 1/16" x 1 1/2" x 3/8"
2nd Designer review: (layout and requested changes only)	01-15-16 KT	Line Screen:	None
PMS Colors Used in File:	Black PMS 185 PMS 298 PMS 298 with diagonal lines Non Varnish		

0.8% Surgiscreen® 0.8+0.2%

For use with Ortho BiVue® System to detect unexpected blood group antibodies / Pour la détection d'anticorps sanguins inattendus avec Ortho BiVue® System / Zum Nachweis von Ortho BiVue® System / Para utilizar con Ortho BiVue® System / Para a detecção de anticorpos inesperados de grupo sanguíneo / Da utilização com Ortho BiVue® System, para detecção de anticorpos incompatíveis / Para utilização com o Ortho BiVue® Irregular / Para detecção de anticorpos de grupos sanguíneos inesperados / For identifying mod blood group antibodies / For detecting mod blood group antibodies / For detecting mod blood group antibodies / For detecting mod blood group antibodies / For detecting mod blood group antibodies


3 x 10 mL

1 1 x 10 mL
2 1 x 10 mL
3 1 x 10 mL

IVD

REF 719102

Ortho BiVue® System for pinching air irregular blood type indicator / Para uso com o Ortho BiVue® System para pinçar o ar irregular blood type indicator / Para uso com o Ortho BiVue® System para pinçar o ar irregular blood type indicator / Para uso com o Ortho BiVue® System para pinçar o ar irregular blood type indicator / Para uso com o Ortho BiVue® System para pinçar o ar irregular blood type indicator

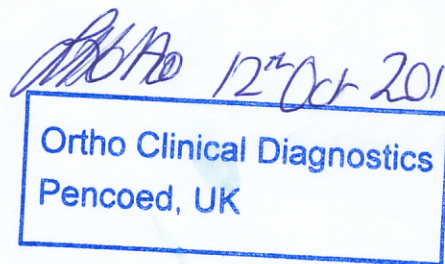


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kim DePaula	SPC Number in OTIS:	SPC544B2
Date File Was Last Modified:	01-14-16	Dimension on SPC:	2-11/16" x 1-1/2" x 3-3/8"
2nd Designer review:	01-15-16 KT	Line Screen:	None
PMS Colors Used in File:		Black PMS 185 PMS 238 Non Varnish	

01-14-16: KD used approved 701-85-003-1CRMU, updated to new component number and made revs per marked up PDF for Crimson PH2 project.
01-15-16 KT signed.

701-80-013-1
Red Cells Carton
France

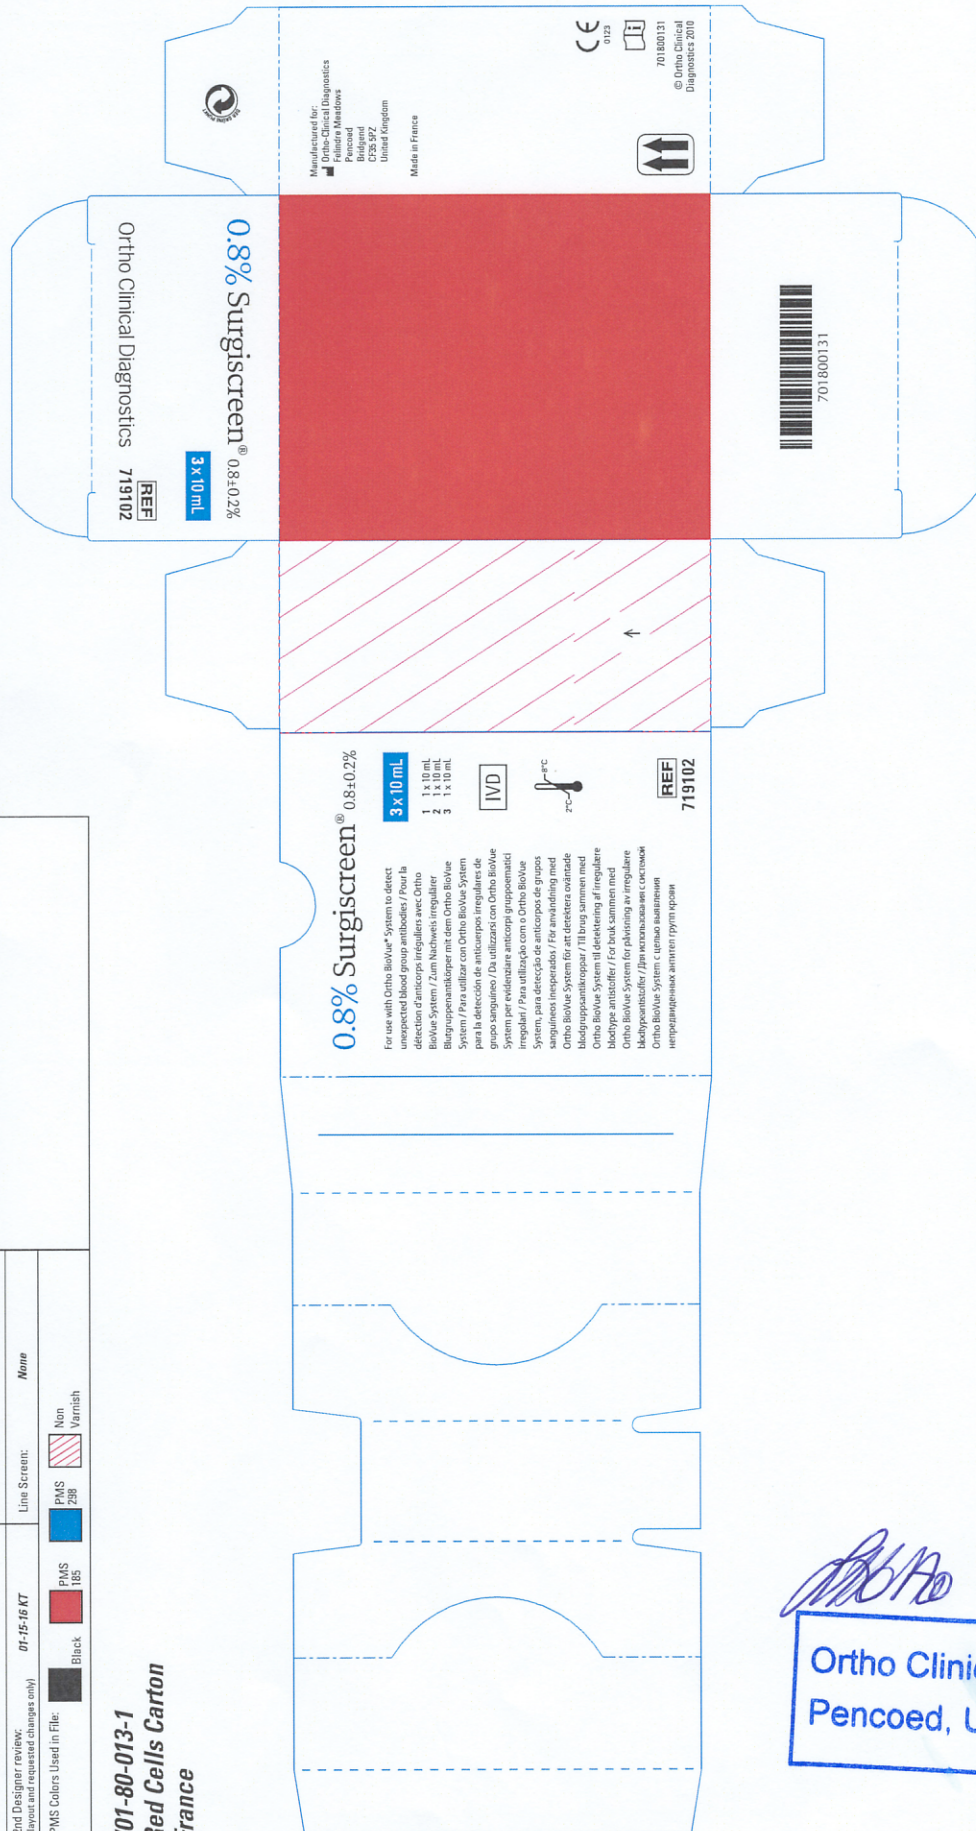

Ortho Clinical Diagnostics
Pencoed, UK
12th Oct 2016