


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kim DePaola	SPC Number in OTIS:	SPC54524	01-12-16: KD used approved 601-80-079-1CRMU, added new component number and made revs per marked up PDF for Crimson PH2 project. 01-13-16 KT signed.
Date File Was Last Modified:	01-12-16	Dimension on SPC:	2.25" x 1.25"	
2nd Designer review: (layout and requested changes only)	01-13-16 KT	Line Screen:	PMS 185 – 30% 85 line screen	
PMS Colors Used in File:	Black PMS 185 PMS 298			

601-80-163-1
Red Cells Label




Rev A 12th Oct 2017

Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kim DePaola	SPC Number in OTIS:	SPC54525	01-12-16: KD used approved 601-80-080-1CRMU, added new component number and made revs per marked up PDF for Crimson PH2 project. 01-13-16 KT signed.
Date File Was Last Modified:	01-12-16	Dimension on SPC:	2.25" x 1.25"	
2nd Designer review: (layout and requested changes only)	01-13-16 KT	Line Screen:	PMS 185 - 30% 85 line screen	
PMS Colors Used in File:	Black	PMS 185	PMS 298	

601-80-164-1
Red Cells Label




PhD 12th Oct 2017
Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kim DePaola	SPC Number in OTIS:	SPC54526	01-12-16: KD used approved 601-80-081-1CRMU, changed to new component number and made revs per marked up PDF for Crimson PH2 project. 01-13-16 KT signed.
Date File Was Last Modified:	01-12-16	Dimension on SPC:	2.25" x 1.25"	
2nd Designer review: (layout and requested changes only)	01-13-16 KT	Line Screen:	PMS 185 - 30% 85 line screen	
PMS Colors Used in File:	Black		PMS 185 PMS 298	

601-80-165-1
Red Cells Label



12th Oct 201
Ortho Clinical Diagnostics
Pencoed, UK

Designer: Who Last Modified File:	Kim DePaola		SFC Number in OTIS:	SFC25483	01-12-16: KD used, approved 371-85-008-1CFRMU, updated to new component number and made new per marked up PDF for Crimson PH2 project. 01-13-16 KT signed.
Date File Was Last Modified:	01-12-16		Dimension on SFC:	3-47/64" X 3-1/64" X 2-3/4"	
2nd Designer review: (review and repeat changes only)	01-13-16 KT		Line Screen:	None	
PMS Colors Used in File:	Black	PMS 185	PMS 298	Non	
				Varnish	

701-80-019-1
Red Cells Carton
France

Ortho Clinical Diagnostics

REF
719111

0.8% BioVue [®] Screen UNTREATED	1-3 1 x 10 mL
0.8% BioVue Screen FICIN TREATED	1-3 1 x 10 mL

6 x 10 mL

Manufactured for:
Ortho-Clinical Diagnostics
Felindre Meadows
Pencoed
Bridgend
CF35 5PZ
United Kingdom

Made in France

Made in France

701800191
© Ortho Clinical
Diagnostics 2010

0.8% BioVue® Screen 0.8±0.2%

0.8% BioVue Screen UNTREATED 1-3 1 x 10 mL

0.8% BioVue Screen FICIN TREATED 1-3 1 x 10 mL

[illegible]

6 x 10 mL

IVD



REF 719111



701800191


Ortho Clinical Diagnostics
Pencoed, UK

12th Oct 2017

OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kim DePaola	SPC Number in OTIS:	SPC54527	01-12-16: KD used approved 601-80-082-1CRMU, added new component number and made revs per marked up PDF for Crimson PH2 project. 01-13-16 KT signed.
Date File Was Last Modified:	01-12-16	Dimension on SPC:	2.25" x 1.25"	
2nd Designer review: (layout and requested changes only)	01-13-16 KT	Line Screen:	PMS 185 - 30% 85 line screen	
PMS Colors Used in File:	Black	PMS 185	PMS 298	

601-80-166-1
Red Cells Label



Ortho Clinical Diagnostics
Pencoed, UK

Steven 12th Oct 2017


Designer Who Last Modified File:	<i>Kim DePaola</i>	SPC Number in OTIS:	<i>SPC54528</i>
Date File Was Last Modified:	<i>01-12-16</i>	Dimension on SPC:	<i>2.25" x 1.25"</i>
2nd Designer review: (layout and requested changes only)	<i>01-13-16 KT</i>	Line Screen:	<i>PMS 185 - 30% 85 line screen</i>
PMS Colors Used in File:			

Mon 12th Oct 2017

OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	<i>Kim DePaola</i>	SPC Number in OTIS:	SPC54529	01-12-16: KD used approved 601-80-084-1CRMU, added new component number and made revs per marked up PDF for Crimson PH2 project. 01-13-16 KT signed.
Date File Was Last Modified:	01-12-16	Dimension on SPC:	2.25" x 1.25"	
2nd Designer review: (layout and requested changes only)	01-13-16 KT	Line Screen:	PMS 185 - 30% 85 line screen	
PMS Colors Used in File:	Black		PMS 298	

601-80-168-1
Red Cells Label





Ortho Clinical Diagnostics
Pencoed, UK

12th Oct 2017

OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kim DePaula	SPC Number in OTIS:	SPC54483	01-12-16 KO used approved 701-85-006 (CRMU) updated to new component number and made new per marked up PDF for Crimson PH2 project. 01-13-16 KT signed.
Date File Was Last Modified:	01-12-16	Dimension on SPC:	3.4784" X 2.184" X 2.34"	
2nd Designer review: (layout and requested changes only)	01-13-16 KT	Line Screen:	None	
PMS Colors Used in File:	Black	PMS 185	PMS 298	Non Varnish

701-80-019-1
Red Cells Carton
France

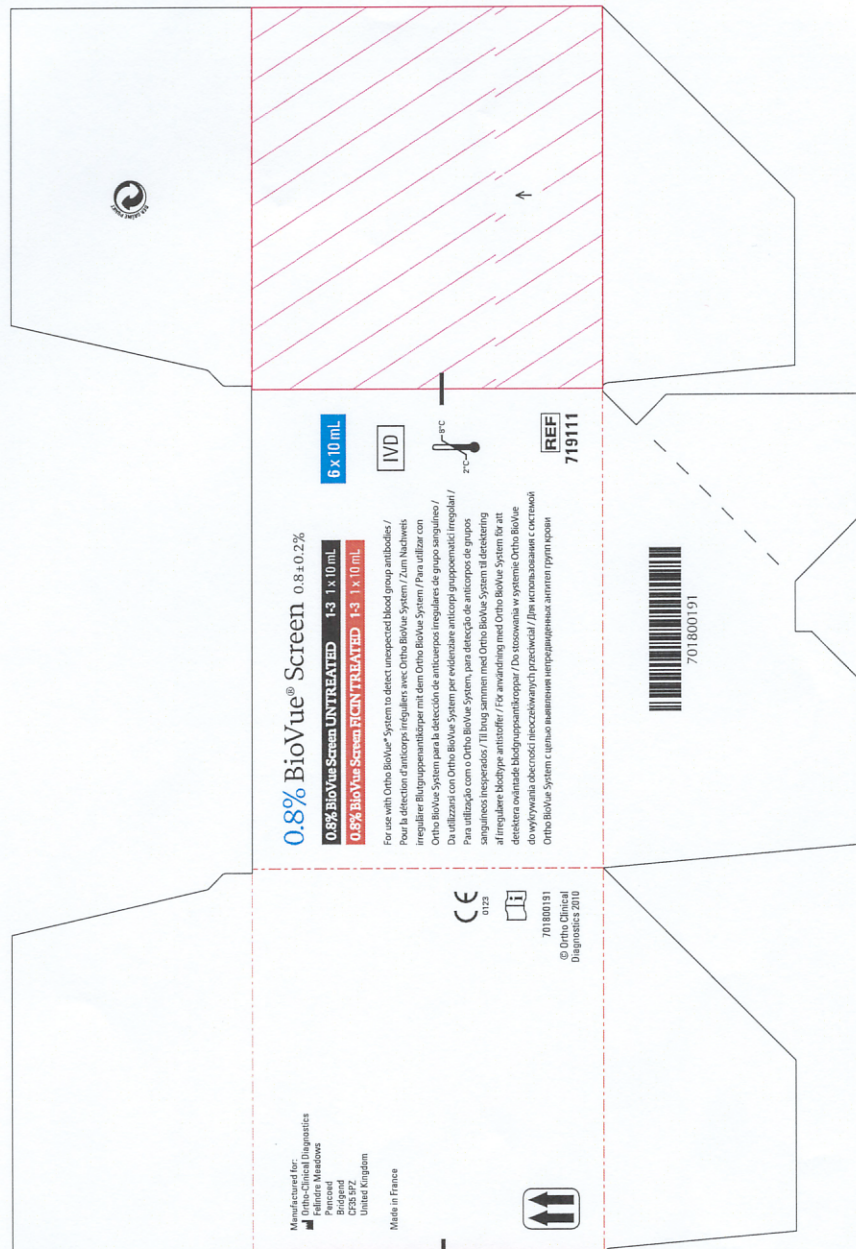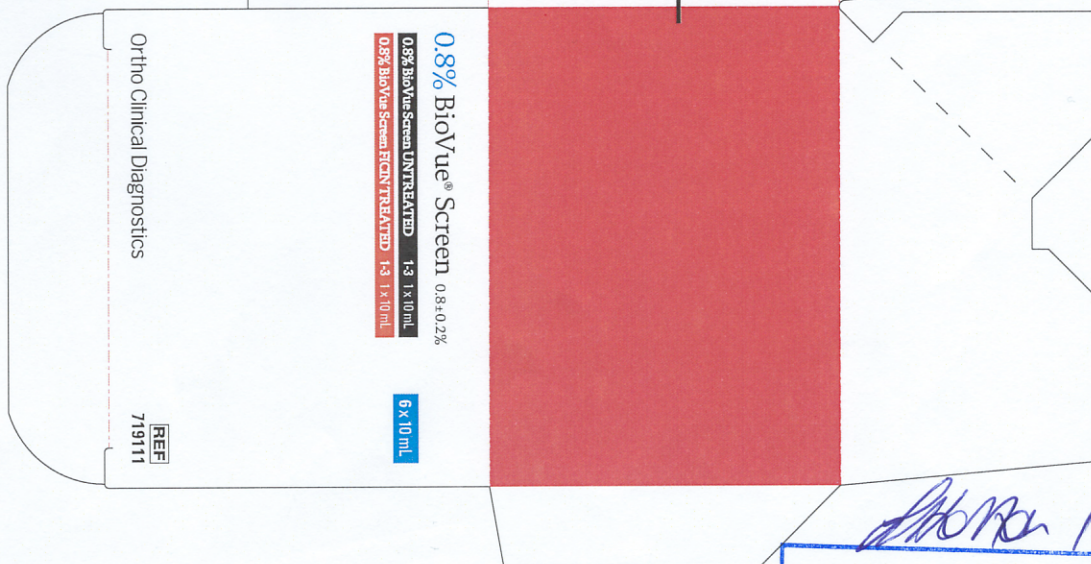

Ortho Clinical Diagnostics
Pencoed, UK

12th Oct 2017