


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kyle Tevlin	SPC Number in OTIS:	SPC50000	LBL 51236	02-19-16 KT used Label154CRMU and made revs for Crimson PH2 per LM markup "BV_Line4_Front_Cassette_Label_Sample_Markup.2-18-16.pdf." (Tailcode does not go on label itself.) 02-19-16: KD signed.
Date File Was Last Modified:	02-19-16	Dimension on SPC:	49.2 mm x 31 mm		
2nd Designer review: (layout and requested changes only)	02-19-16:KD	Line Screen:	None		
PMS Colors Used in File:	 Black	 PMS 185	 PMS 298		

**Label154-2
BioVue Cassette Front Label
for Pencoed**

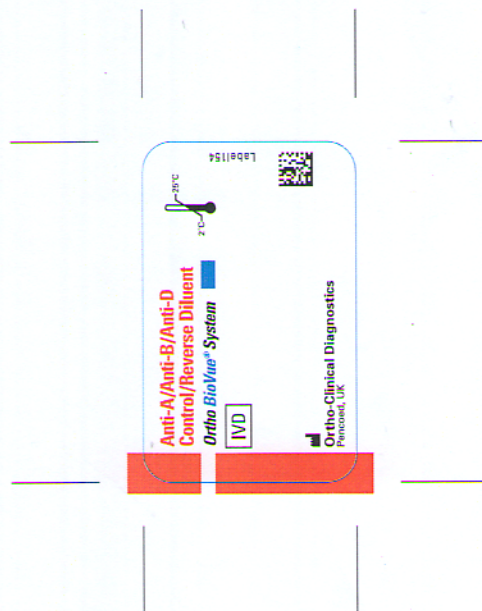

Ortho Clinical Diagnostics
Pencoed, UK

5th Oct 2017


OCD Mechanical Info.

FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File:	2/25/14.LC for PL	Designer Who First Created File:	Kim DePaola
Date Pkg. Engineering Approved File:	2/21&24/14.MC.KD	Date File Was Last Modified:	12/24/13
Dimension on Specification:	49.2 mm x 31 mm	Designer Who Last Modified File:	Kyle Tevlin
Drawing # NA	LBL NA	Designer review:	1/7/14.KD
Line Screen:	None		
PMS Colors Used in File: Black PMS 123 PMS 298 PMS 429			

OTHER: 12/24/13 KT used 606-30-002-1 as base, using new component code and data matrix for Pencoed. Placed new slug.
1/7/14: KD signed.
2/27/14: KD added approval dates & locked file.

Label156 BioVue Cassette Label Back for Pencoed

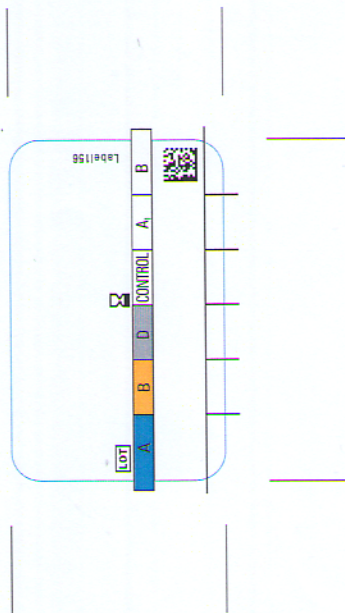

Ortho Clinical Diagnostics
Pencoed, UK

Handwritten signature 5th Oct 2017

OCD Mechanical Info.

FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File: 2/25/14.LC for PL	Designer Who First Created File: Kim DePaola	OTHER: 12/24/13: KT used 604-30-003-4 as base, using new component code for Pencoed. Also added data matrix, and deleted FOR EXPORT ONLY and arrow in GS1 area. Updated slug and updated dimensions into cm. 1/7/14: KD signed. 2/27/14: KD entered approval dates & locked file.
Date Pkg. Engineering Approved File: 2/21&24/14.MC.KD	Date File Was Last Modified: 12/24/13	
Dimension on Specification: 16.51cm x 14.6cm	Designer Who Last Modified File: Kyle Tevlin	
Drawing # N/A	Designer review: 1/7/14.KD (layout and requested changes only)	
Line Screen: N/A		
PMS Colors Used in File: Black		


Label196
BioVue Shipper Label
for Pencoed

Ortho Clinical Diagnostics
Pencoed, UK

57th Oct 2017

Anti-A (AB01) / Anti-B (AB02) / Anti-D (Anti-RH1) /
Control / Reverse Diluent
抗 A / 抗 B / 抗 D / 质控 / 反定型稀释液
Ortho BioVue® System

Blue box does not print.
Indicates GS1 area.

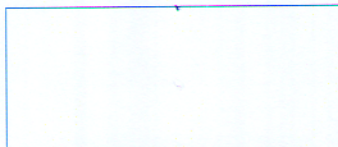

IVD



© Ortho-Clinical
Diagnostics, Inc. 2002
Label196

CE
0123



REF
707100