


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kyle Tevlin	SPC Number in OTIS:	SPC50400	LBL 51233	02-19-16 KT used Label144CRMU and made revs for Crimson PH2 per LM markup "BV_Line4_Front_Cassette_Label_Sample_Markup.2-18-16.pdf." (Tailcode does not go on label itself.) 02-19-16: KD signed.
Date File Was Last Modified:	02-19-16	Dimension on SPC:	49.2 mm x 31 mm		
2nd Designer review: (layout and requested changes only)	02-19-16:KD	Line Screen:	None		
PMS Colors Used in File:	 Black  PMS 185  PMS 246				

Label144-2 BioVue Cassette Front Label for Pencoed

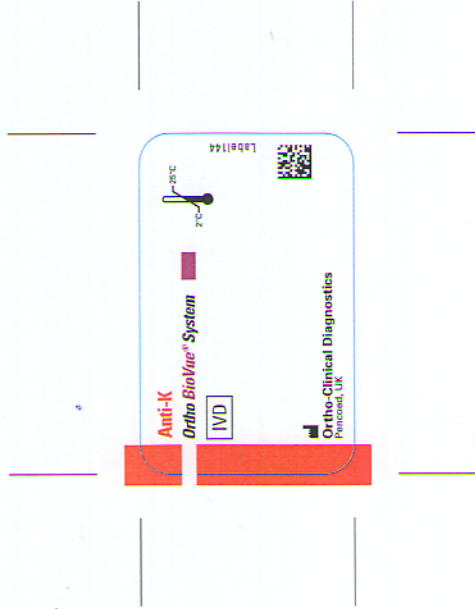

Ortho Clinical Diagnostics
Pencoed, UK


Revised 5th Oct 2017

OCD Mechanical Info.

FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File:		07/07/14 CC		OTHER: 4/4/14: KD used 606-30-055-1 as base, assigned new Pencoed component number Label145, added new dm code, added new slug and updated slug info. 04/07/14 CR signed 07/08/14 CR entered CC and Eng approval dates
Date Pkg. Engineering Approved File:		07/07/14 MC SF		
Dimension on Specification:		49.2 mm x 31 mm		
Drawing # NA	LBL NA			
Line Screen: None				
PMS Colors Used in File:				
Black		PMS 1505		

Label 145
BioVue Cassette Label Back
Pencoed

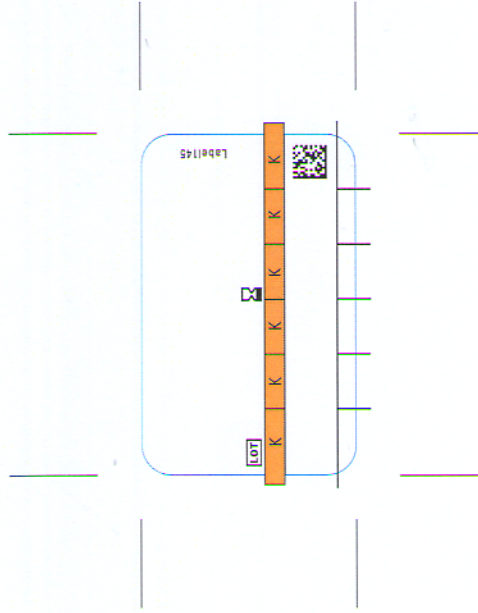

Ortho Clinical Diagnostics
Pencoed, UK

5th Oct 2017

OCD Mechanical Info.

FOR OCD USE ONLY - REFER TO SPECIFICATION


Date Copy Created Approved File:	7/8/14 CC for LC	Designer Who First Created File:	Kim DuPaula
Date Pkg. Engineering Approved File:	7/7/14 M.C.S.F	Date File Was Last Modified:	4/4/14
Dimension on Specification:	20.32 cm x 7.62 cm	Designer Who Last Modified File:	Kim DuPaula
Drawing #	NA	Designer review:	04/07/14 CR
Line Screen:	None	(layout and requested changes only)	
PMS Colors Used in File:	Black		

4/4/14: KD used OCD Revision number 004-30-024-2 as base template and added new Pencoeed number Label216, added new data matrix code, removed "FOR EXPORT ONLY", removed GSI arrow and added new slug, KD changed size of label to be slightly smaller and in centimeters per Email from Pencoeed.
04/07/14 CR signed
7/8/14: KD added approval dates & locked file.

Label 216
BioVue Shipper Label
Pencoeed

Anti-K
Ortho BioVue® System

IVD

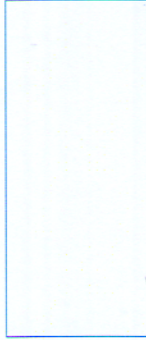

Ortho Clinical
Diagnostics, Inc. 2002
Label216



CE 0123

REF
707117

Blue box does not print.
← Indicates GSI area.

Ortho Clinical Diagnostics
Pencoeed, UK

5th Oct 2017