


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kyle Towlin	SPC Number in OTIS:	SPC50040	LBL 51230	02-19-16 KT used Label132CRMU and made revs for Crimson PH2 per LM markup "BY_Lined_Front_Cassette_Label_Sample_Markup-2-18-16.pdf." (Tailcode does not go on label itself.) 02-19-16: KD signed.
Date File Was Last Modified:	02-19-16	Dimension on SPC:	49.2 mm x 31 mm		
2nd Designer review: (layout and requested changes only)	02-19-16 KD	Line Screen:	None		
PMS Colors Used in File:	Black PMS 185 PMS 2572				

Label132-2 BioVue Cassette Front Label for Pencoed

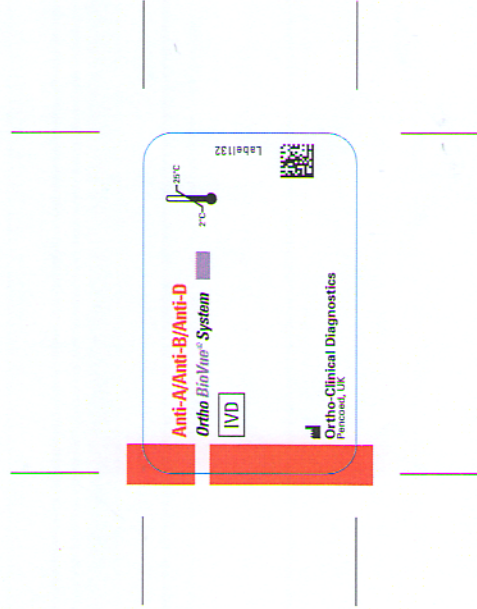

Ortho Clinical Diagnostics
Pencoed, UK


MDA 574 Oct 2017

OCD Mechanical Info.

FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File:	07/07/14 CC			OTHER: 03/04/14 CR used 606-30-038-1 as base Made revs per markedup PDF 3/6/14 took space between Label and 134 per KT review 3/7/14 KT signed. 07/08/14 CR entered CC and Eng approval dates
Date Pkg. Engineering Approved File:	07/07/14 MC SF			
Dimension on Specification:	49.2 mm x 31 mm			
Drawing # N/A	LBL N/A			
Line Screen: NA				
PMS Colors Used in File:				
Black PMS 298 PMS 123 PMS 429				
Designer Who First Created File:	Candace Figueroa			
Date File Was Last Modified:	03/06/14			
Designer Who Last Modified File:	Candace Rechsteiner			
Designer review: (layout and requested changes only)	3/7/14 KT			

Label134 BioVue Cassette Back Label for Pencoed

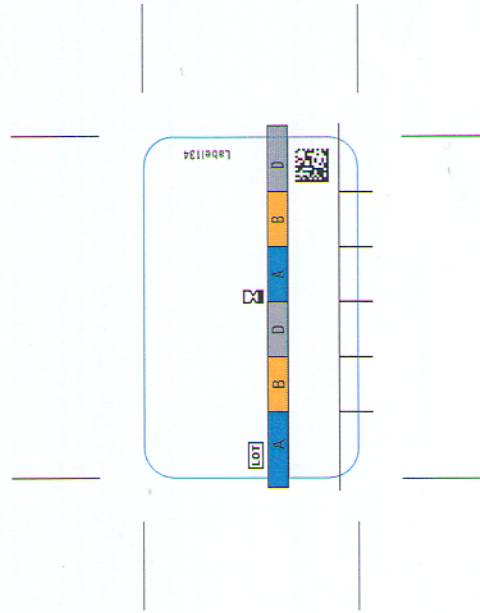

Ortho Clinical Diagnostics
Pencoed, UK

MDM
5th Oct 2017


OCD Mechanical Info.

Date Copy Control Approved File:	7/9/14 CE for LC	Designer Who First Created File:	Kim DePaula	OTHER: CR used 604-30-019-3 as base. Made revs per marked up PDF. 3/6/14 CR fixed LBL. Review date, and tailcode shown per KT review 3/7/14 KT signed. 7/9/14 KD entered approval dates & locked file.
Date Pkg. Engineering Approved File:	7/7/14 MC-SF	Date File Was Last Modified:	3/6/14	
Dimension on Specification:	20.32cm x 7.62cm	Designer Who Last Modified File:	Candace Bachsteiner	
Drawing #	N/A	Designer review: (layout and requested changes only)	3/7/14 KT	
Line Screen:	N/A			
PMS Colors Used in File:	Black			


**Label166
Shipper Label
for Pencoed**

Anti-A (Anti-AB01) / Anti-B (Anti-AB02) / Anti-D (Anti-RH1)
抗 A / 抗 B / 抗 D
Ortho BioVue® System

IVD

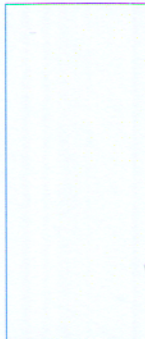

Blue box does not print.
← Indicates GS1 area.



Ortho Clinical Diagnostics
Pencoed, UK

MDA 5th Oct 2017