


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kyle Tevlin	SPC Number in OTIS:	SPC50040	LBL 51224	02-19-16 KT used Label104CRMU and made revs for Crimson PH2 per LM markup "BV_Line4_Front_Cassette_Label_Sample_Markup.2-18-16.pdf." (Tailcode does not go on label itself.) 02-19-16: KD signed.
Date File Was Last Modified:	02-19-16	Dimension on SPC:	49.2 mm x 31 mm		
2nd Designer review: (layout and requested changes only)	02-19-16:KD	Line Screen:	None		
PMS Colors Used in File:	 Black	 PMS 185	 PMS 429		

Label104-2 BioVue Cassette Front Label for Pencoed

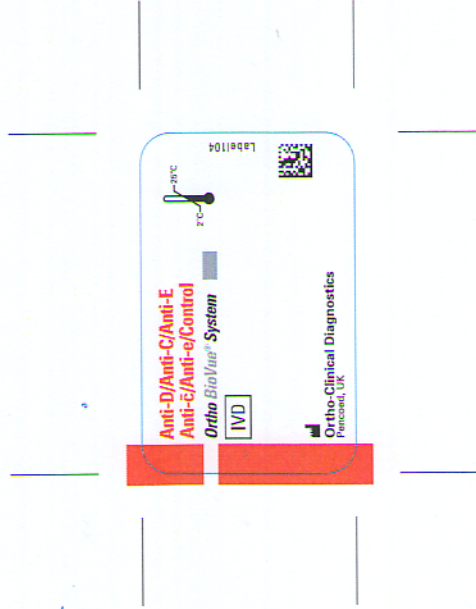


5th Oct 2017

Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info. **FOR OCD USE ONLY - REFER TO SPECIFICATION**

Date Copy Control Approved File:	07/07/14 CC	Designer Who First Created File:	Colleen Miller
Date Pkg. Engineering Approved File:	07/07/14 MC SF	Date File Was Last Modified:	3/3/14
Dimension on Specification:	49.2 mm x 31 mm	Designer Who Last Modified File:	Kyle Tavlin
Drawing #	N/A	Designer review:	03/04/14 CR
Line Screen:	NA	(layout and requested changes only)	
PMS Colors Used in File: Black PMS 429 PMS 224 PMS 153 PMS 2572 PMS 352			
OTHER: 3/3/14 KT used 606-30-010-1 as base, using new component code and data matrix for Pencoed. Changed dimensions in slug to mm. 03/04/14 CR signed 07/08/14 CR entered CC and Eng approval dates			

Label106 **BioVue Cassette Back Label** **for Pencoed**

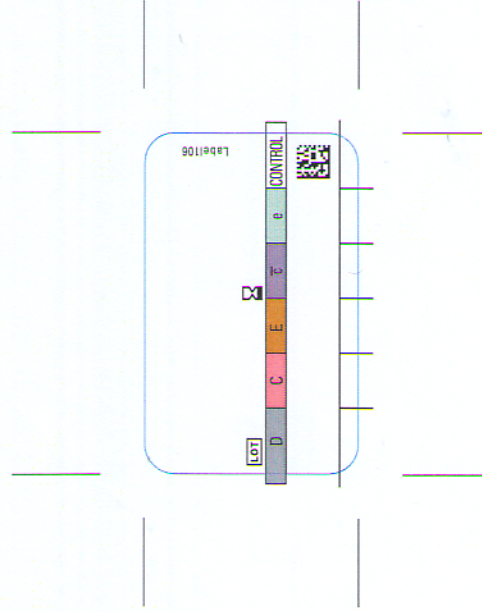

Marked 5th Oct 2017

Ortho Clinical Diagnostics
 Pencoed, UK


OCD Mechanical Info. FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File:	7/8/14.CC for LC	Designer Who First Created File:	Kim DePaola	OTHER: 32714 KT used 604-30-006-2 as base, using new component code for Pencoed. Deleted FOR EXPORT ONLY and arrow in GSI area, and added data matrix. Updated slug and changed size from 8" x 3" to 20.32cm x 7.62cm per AG
Date Pkg. Engineering Approved File:	7/7/14.MG.SF	Date File Was Last Modified:	3/2/14	03/04/14 CE signed
Dimension on Specification:	20.32cm x 7.62cm	Designer Who Last Modified File:	Kyle Twolin	7/8/14 KD entered approval dates & tested file.
Drawing # N/A	131, MA	Designer reviewer: Report and requested changes only	03/04/14 CR	
Line Screen: MA				
PMS Colors Used in File:	Black			


Label 184
Shipper Label
for Pencoed

Anti-D / Anti-C / Anti-E / Anti-ε / Anti-e / Control
Ortho BioVue[®] System

IVD

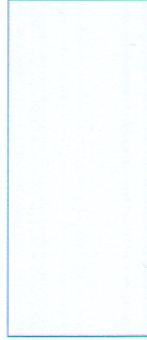

Blue box does not print.
← Indicates GSI area.



5th Oct 2017

Ortho Clinical Diagnostics
Pencoed, UK