


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kyle Tevlin	SPC Number in OTIS:	SPC54000	LBL 51223	02-19-16 KT used Label116C.RML and made revs for Crimson PH2 per LM markup "BV_Line4_Front_Cassette_Label_Sample_Markup 2-18-16.pdf." (Tailcode does not go on label itself.) 02-19-16: KD signed.
Date File Was Last Modified:	02-19-16	Dimension on SPC:	49.2 mm x 31 mm		
2nd Designer review: (layout and requested changes only)	02-19-16.KD	Line Screen:	None		
PMS Colors Used in File:	Black PMS 185				

Label116-2 BioVue Cassette Front Label for Pencoed

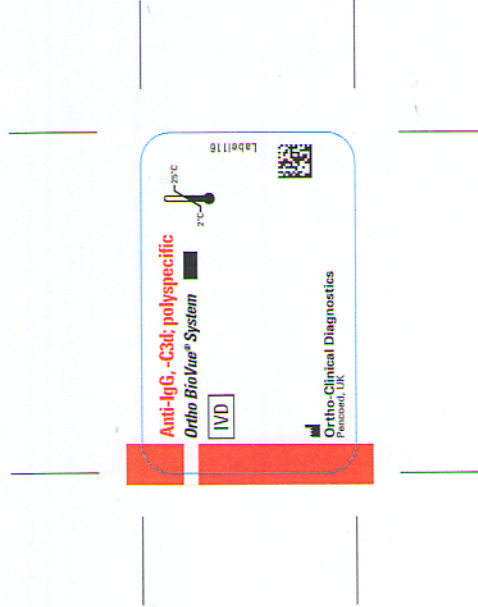

Steven 5th Oct 2017


Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info.

FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File:	01/30/14 LC			OTHER: KT used 606-30-023-1 as base, using new component code and data matrix for Pencoed. 12/12/13 CR signed and entered dimensions in mm on file 01/31/14 CR entered CC and Eng approval dates, locked file, made PDF
Date Pkg. Engineering Approved File:	01/30/14 MC JM			
Dimension on Specification:				
49.2 mm x 31 mm				
Drawing #	N/A	LBL N/A		
Line Screen: NA				
PMS Colors Used in File:				
Black PMS 421				
Designer Who First Created File:		Colleen Miller		
Date File Was Last Modified:		12/11/13		
Designer Who Last Modified File:		Kyle Tovlin		
Designer review: (layout and requested changes only)		12/12/13 CR		

Label118
BioVue Cassette Back Label
for Pencoed

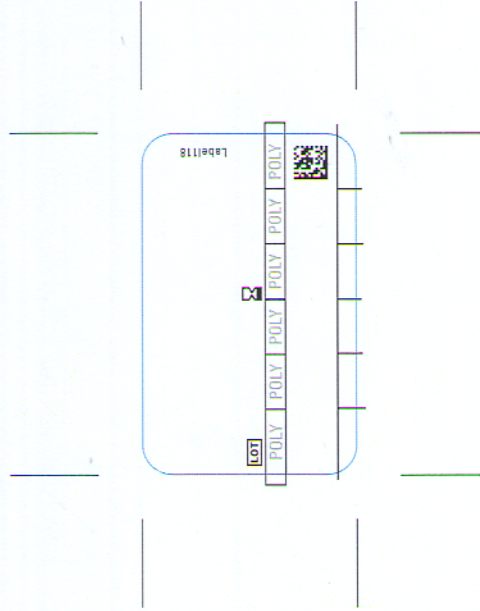

Ortho Clinical Diagnostics
Pencoed, UK

Ortho Clinical Diagnostics
 Pencoed, UK

OCD Mechanical Info. FOR OCD USE ONLY - REFER TO SPECIFICATION


Data Copy Control Approved File:	1/30/14 LC	Designer Who First Created File:	Kim DePaula
Date Pkg. Engineering Approved File:	1/30/14 MC JM	Date File Was Last Modified:	12/13/13
Dimension on Specification:	20.32cm x 7.62cm	Designer Who Last Modified File:	Kyle Tevlin
Drawing # N/A	LBL 50095	Designer review:	12/13/13 KD
Line Screen: NA		(layout and requested changes only)	
PMS Colors Used in File:			
	Black		

OTHER: KT used 694-30-011-3 as base, using new component code for Pencoed. Also added data matrix, and deleted FOR EXPORT ONLY and arrow in GS1 area.
 Updated slug.
 12/13/13 KT changed size from 8" x 3" to 20.32cm x 7.62cm per AG email
 12/13/13 KD signed.
 01/28/14 CK signed and entered EC and Eng approval dates and made PDF

Label176
 Shipper Label
 for Pencoed

Anti-IgG, -C3d; polyspecific
 抗 IgG、抗 C3d 多特异性
 Ortho BioVue® System

IVD

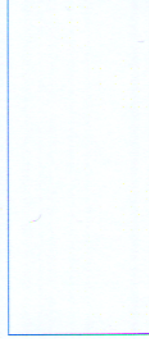

Blue box does not print.
 ← Indicates GS1 area.



©Ortho-Clinical
 Diagnostics, Inc. 2002
 Label176



CE 0123

REF 707350

Shipped 5th Oct 2017

Ortho Clinical Diagnostics
 Pencoed, UK