


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kyle Tevlin	SPC Number in OTIS:	SPC54040	LBL 51228	02-19-16 KT used Label124CRMU and made revs for LM markup "BV_Line4_Front_Cassette_Label_Sample_Markup.2-18-16.pdf." (Tailcode does not go on label itself.) 02-19-16: KD signed.
Date File Was Last Modified:	02-19-16	Dimension on SPC:	49.2 mm x 31 mm		
2nd Designer review: (layout and requested changes only)	02-19-16.KD	Line Screen:	None		
PMS Colors Used in File:					
Black PMS 185 PMS 352					

Label124-2 BioVue Cassette Label Front for Pencoed

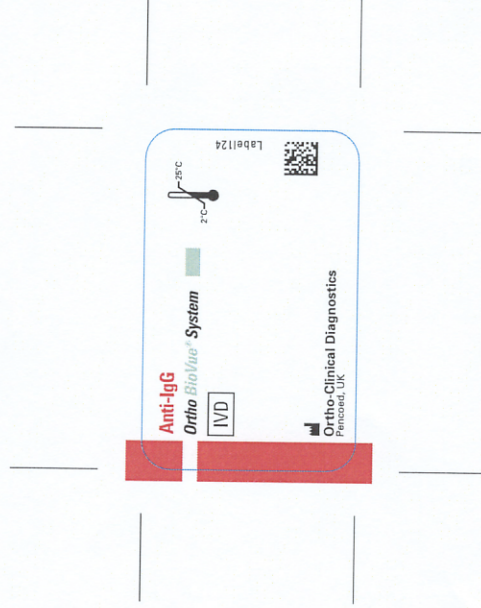

BBM 5th Oct 2017


Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info.

FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File:	02/04/14 LC for PL		Designer Who First Created File:	Kim DePaola	OTHER: 12/16/13: KD used 606-30-030-1 as base and added new Pencoed component number and new datamatrix code per markup from R. Parente for Pencoed. 12/19/13 KT signed. 02/04/14 CR entered CC and Eng approval dates, locked file and made PDF
Date Pkg. Engineering Approved File:	02/03/14 MC 02/04/14 BB		Date File Was Last Modified:	12/16/13	
Dimension on Specification:	49.2 mm x 31 mm		Designer Who Last Modified File:	Kim DePaola	
Drawing # NA	LBL NA		Designer review: (layout and requested changes only)	12/19/13 KT	
Line Screen:	None				
PMS Colors Used in File:					
		Black		PMS 339	
				PMS 352	

Label126 BioVue Cassette Label Back for Pencoed

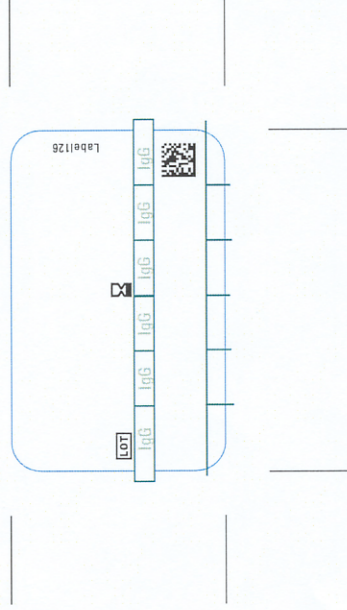

Done 5th Oct 2017

Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info.


FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File: 02.04.14 LC for PL	Designer Who First Created File: Kim DePaola	OTHER: 12/19/13: KD used OCD Raritan number 604-30-016-4 as base template and added new Pencoed number Label186, added new datamatrix code, removed "FOR EXPORT ONLY", removed GS1 arrow and added new slug. KD changed size to be in centimeters instead of inches per Pencoed. 12/19/13 KT signed. 02/04/14 CR entered CC and Eng approval dates, locked file and made PDF
Date Pkg. Engineering Approved File: 02/03/14 MC 02/04/14 BB	Date File Was Last Modified: 12/19/13	
Dimension on Specification: 16.51 cm x 14.6 cm	Designer Who Last Modified File: Kim DePaola	
Drawing # NA	Line Screen: None	
PMS Colors Used in File: Black	Designer review: (layout and requested changes only) 12/19/13 KT	

Label186
BioVue Shipper Label
for Pencoed

Anti-IgG
抗 IgG
Ortho BioVue® System

Blue box does not print.
Indicates GS1 area. →

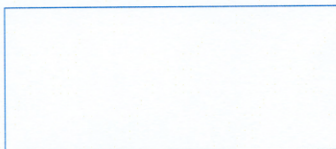

IVD



© Ortho-Clinical
Diagnostics, Inc. 2002
Label186



REF
707400

5th Oct 2017

Ortho Clinical Diagnostics
Pencoed, UK