


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kyle Tevlin	SPC Number in OTIS:	SPC54040	LBL51229	02-19-16 KT used Label128CRMU and made revs for Crimson PH2 per LM markup "BV Line4 Front Cassette Label Sample Markup.2-18-16.pdf." (Tailcode does not go on label itself.) 02-19-16: KD signed.
Date File Was Last Modified:	02-19-16	Dimension on SPC:	49.2 mm x 31 mm		
2nd Designer review: (layout and requested changes only)	02-19-16.KD	Line Screen:	None		
PMS Colors Used in File:	Black PMS 185				

Label128-2
BioVue Cassette Label Front
for Pencoed

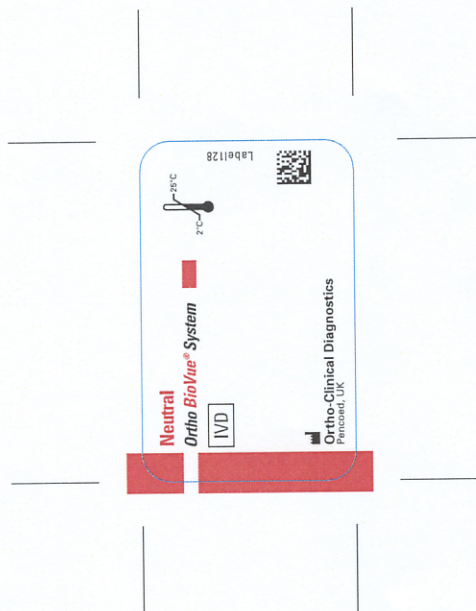

Marked 5th Oct 2017


Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info.

FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File: 07/07/14 CC		OTHER: 3/3/14: KD used 606-30-034-1 as base template, changed to new Label number, placed new DM code, added new slug and made dimensions metric. 3/6/14 KT signed. 07/08/14 CR entered CC and Eng approval dates
Date Pkg. Engineering Approved File: 07/07/14 MC SF		
Dimension on Specification: 49.2 mm x 31 mm		
Drawing # NA	LBL NA	
Line Screen: None		
PMS Colors Used in File: Black PMS 185 PMS 1765		
Designer Who First Created File: Kim DePaola		
Date File Was Last Modified: 3/3/14		
Designer Who Last Modified File: Kim DePaola		
Designer review: (layout and requested changes only)		3/6/14 KT

Label130 BioVue Cassette Label Back for Pencoe

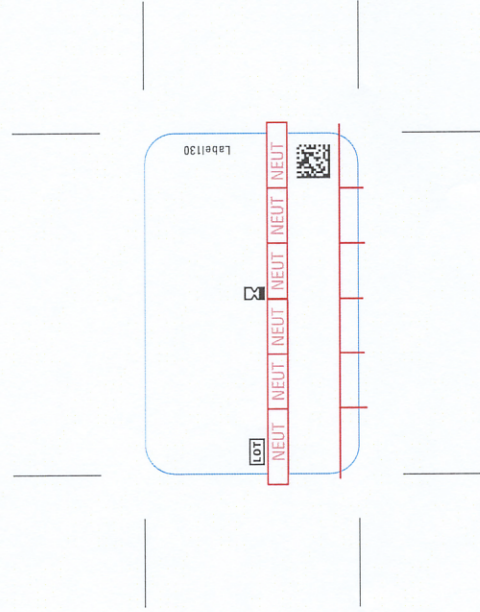

Order 5th Oct 2017


Ortho Clinical Diagnostics
Pencoe, UK

OCD Mechanical Info. FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File:	7/8/14.CC for LC	Designer Who First Created File:	Kim DePaola	3/4/14, KD used OCD Revision number 604-30-0172 as base template and added Ortho Clinical Diagnostics, Inc. logo and removed "FOR EXPORT ONLY" text. 7/8/14, KD added GS1 barcode and added "Label Size of 36/14 KT signed." 7/8/14, KD entered approval dates & locked file.
Date Pkg. Engineering Approved File:	7/7/14.Mc.SF	Date File Was Last Modified:	3/4/14	
Dimension on Specification:	20.32 cm x 7.62 cm	Designer Who Last Modified File:	Kim DePaola	
Drawing # NA	LBL WA	Designer review: (layout and request changes only)	3/6/14 KT	
Line Screen: None				
PMS Colors Used in File:	Black			

Label202
BioVue Shipper Label
for Pencoed

Neutral
Ortho BioVue® System

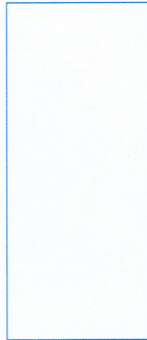

Blue box does not print.
← Indicates GS1 area.



© Ortho-Clinical
Diagnostics, Inc. 2002
Label202



0123



707650

Done 5th Oct 2017

Ortho Clinical Diagnostics
Pencoed, UK