


OCD Mechanical Info. – FOR INTERNAL USE ONLY

Designer Who Last Modified File:	Kyle Tevlin	SPC Number in OTIS:	SPC54040	LBL 51229	02-19-16 KT used Label128CRMU and made revs for Crimson PH2 per LM markup "BV Line4_Front_Cassette_Label_Sample_Markup.2-18-16.pdf." (Tailcode does not go on label itself.) 02-19-16: KD signed.
Date File Was Last Modified:	02-19-16	Dimension on SPC:	49.2 mm x 31 mm		
2nd Designer review: (layout and requested changes only)	02-19-16.KD	Line Screen:	None		
PMS Colors Used in File:	Black				

Label128-2
BioVue Cassette Label Front
for Pencoed

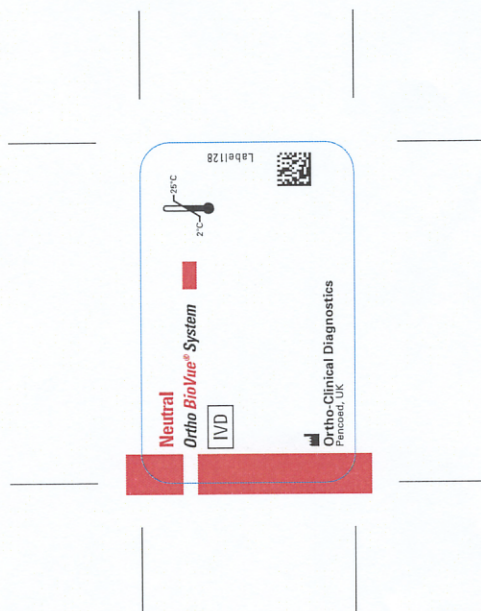

Ortho 5th Oct 2017


Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info.

FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File: 07/07/14 CC		OTHER: 3/3/14: KD used 606-30-034-1 as base template, changed to new Label number, placed new DM code, added new slug and made dimensions metric. 3/6/14 KT signed. 07/08/14 CR entered CC and Eng approval dates
Date Pkg. Engineering Approved File: 07/07/14 MC SF		
Dimension on Specification: 49.2 mm x 31 mm		
Drawing # NA	LBL NA	
Line Screen: None		
PMS Colors Used in File:		Designer Who First Created File: Kim DePaola Date File Was Last Modified: 3/3/14 Designer Who Last Modified File: Kim DePaola Designer review: (layout and requested changes only) 3/6/14 KT
Black PMS 185 PMS 1785		

Label130 BioVue Cassette Label Back for Pencoed

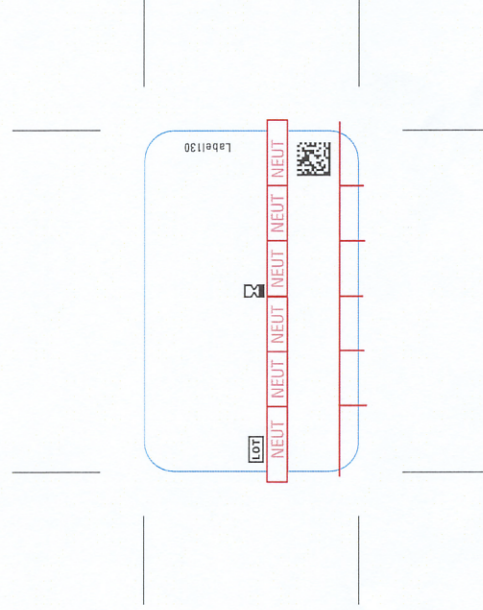

Ortho 5th Oct 2017

Ortho Clinical Diagnostics
Pencoed, UK

OCD Mechanical Info.

FOR OCD USE ONLY - REFER TO SPECIFICATION

Date Copy Control Approved File:	7/8/14.CC for LC	Designer Who First Created File:	Kim DePaola	3/4/14: KD used OCD Revision number 604-30-018-3 as base template and added new Pencoed number Label204, added new datamatrix code, removed "FOR EXPORT ONLY", removed GS1 arrow and added new slug. KD changed size to be in centimeters instead of inches per Pencoed. 3/5/14 KT signed. 7/8/14: KD entered approval dates & locked file.
Date Pkg. Engineering Approved File:	7/7/14.MC.SF	Date File Was Last Modified:	3/4/14	
Dimension on Specification:	16.51 cm x 14.6 cm	Designer Who Last Modified File:	Kim DePaola	
Drawing # NA	LBL NA	Designer review: (layout and requested changes only)	3/5/14 KT	
Line Screen: None				
PMS Colors Used in File:	Black			



Label204
BioVue Shipper Label
for Pencoed

Ortho Clinical Diagnostics
Pencoed, UK

Sharon 5th Oct 2017

Neutral
Ortho BioVue® System

Blue box does not print.
Indicates GS1 area. →

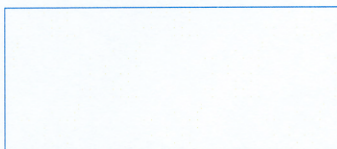

© Ortho-Clinical
Diagnostics, Inc. 2002
Label204

CE 0123  REF 707680